

User Manual

Manuel d'utilisation

Manual de usuario


Gebrauchsanleitung

Manuale dell'utente

(pH) FT11

(TDS) FT34 FT36


(EC) FT33 FT35

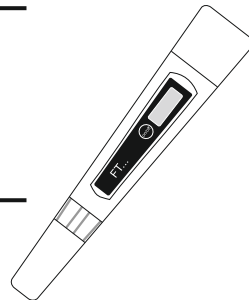


Inverkehrbringer / Distributed by: Water-i.d. GmbH • Daimlerstr. 20 • D-76344 Eggenstein • www.water-id.com

	FT11	FT34	FT36	FT33	FT35
Range	0.0-14.0 pH	0-1999 ppm 0.0-1.999 ppt)	(0-10000 ppm) 0.00-10.00 ppt	0-1999 µS/cm (0-1.999 mS/cm)	(0-19990 µS/cm) 0.00 - 19.99 mS/cm
Resolution	0.1 pH	1 ppm	0.01 ppt	1 µS/cm	0.01 mS/cm
Accuracy	+/- 0.1 pH	+/- 2% FS	+/- 2% FS	+/- 2% FS	+/- 2% FS
Calibration	manual	manual	manual	manual	manual
Temp. Comp.	---	automatic 0 - 50° C β = 2%/°C	automatic 0 - 50° C β = 2%/°C	automatic 0 - 50° C β = 2%/°C	automatic 0 - 50° C β = 2%/°C
Battery Type	3 x 1.5 V	4 x 1.5 V	4 x 1.5 V	4 x 1.5 V	4 x 1.5 V
Batt. Life	~ 1000 h	~250 h	~250 h	~250 h	~250 h
Environment	0 - 50° C RH 100%	0 - 50° C RH 100%	0 - 50° C RH 100%	0 - 50° C RH 100%	0 - 50° C RH 100%

Calibration

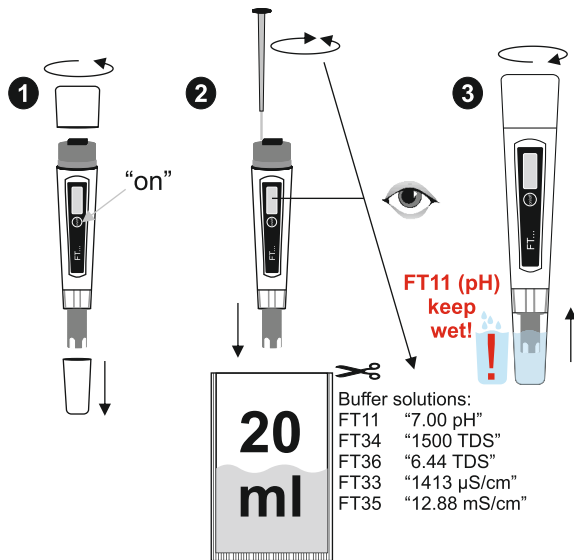

Use

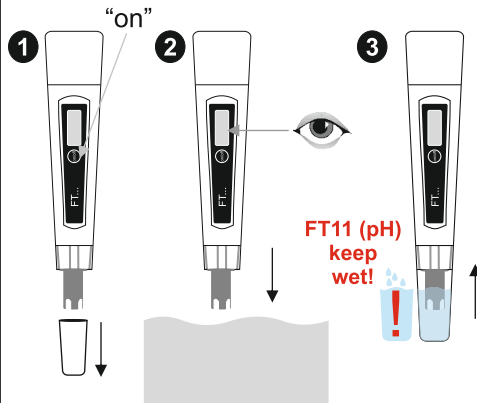

Battery

